





Pulsewave[®] Quick Start Guide

1


Contents

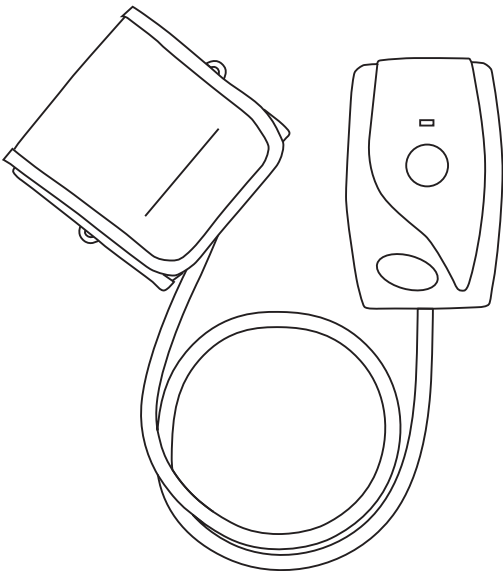

Pulsewave® PAD
(Pulse Acquisition Device)
with Inflatable Wrist Cuff

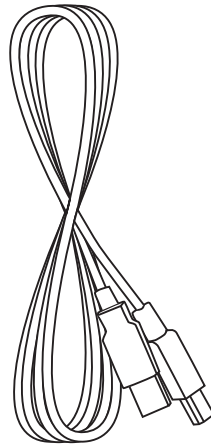

USB cable

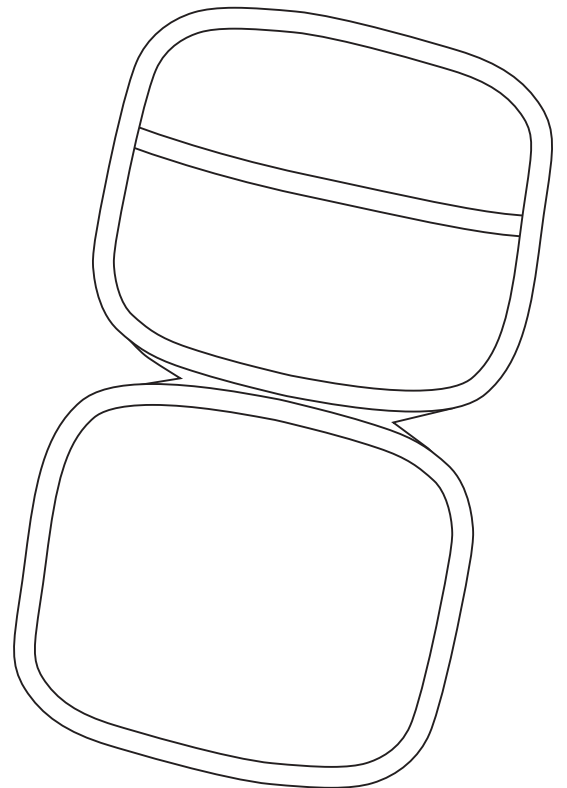


Carrying Pouch

2

Connect


Connect USB cable to the Pulsewave® device.

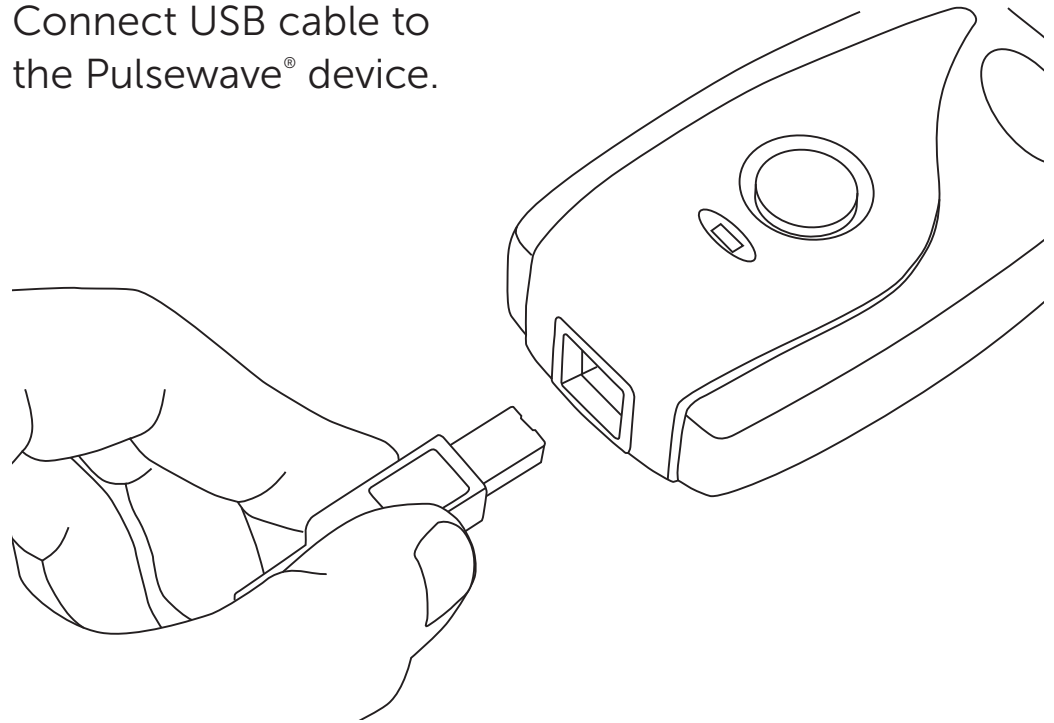

3

Connect


Connect USB
cable to your
computer.

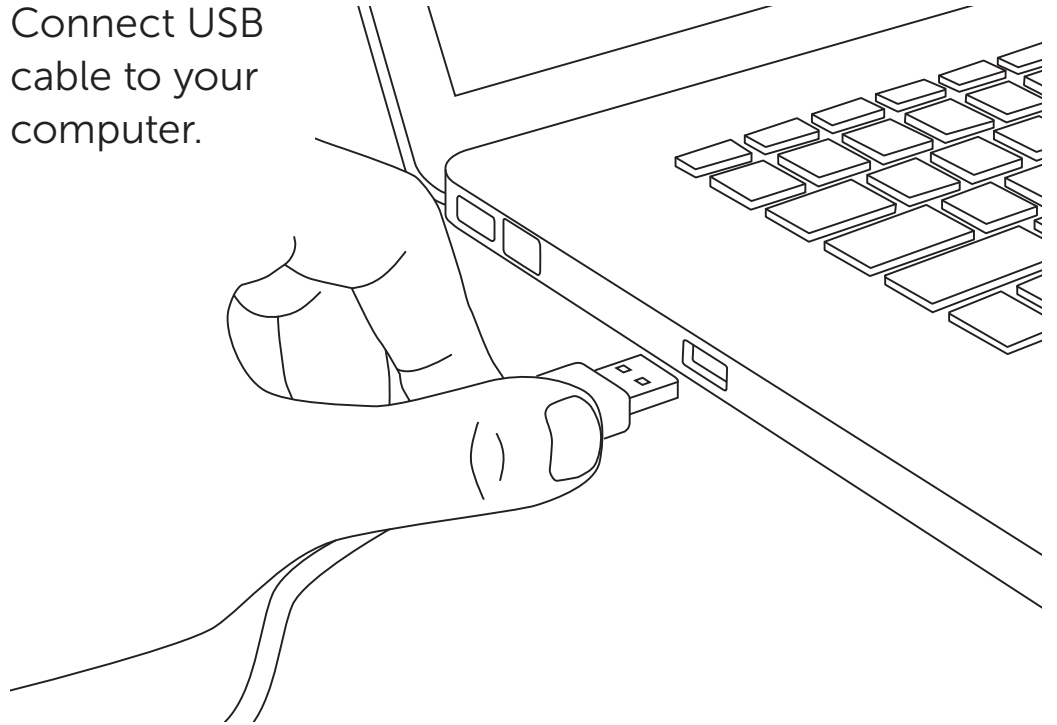

4

Register


If you have your user name and password, please skip to step 5. Otherwise, please visit www.cloudDX.com and create your account.

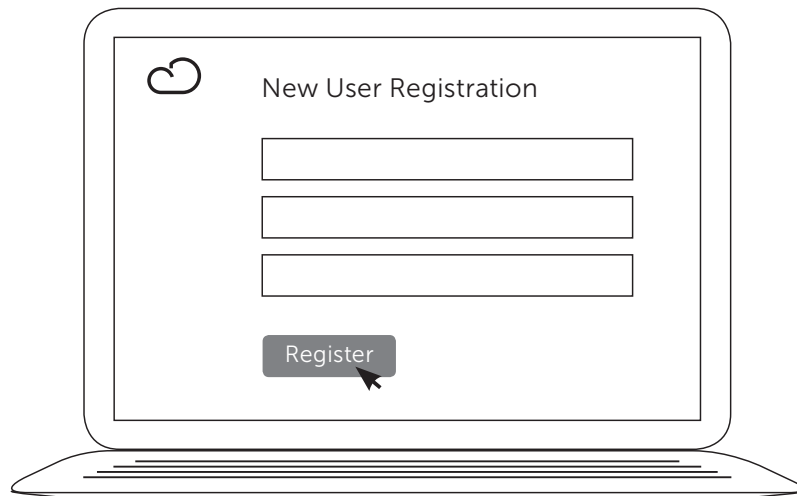

5

Log in

Please visit www.clouddx.com and log in with your user name and password.

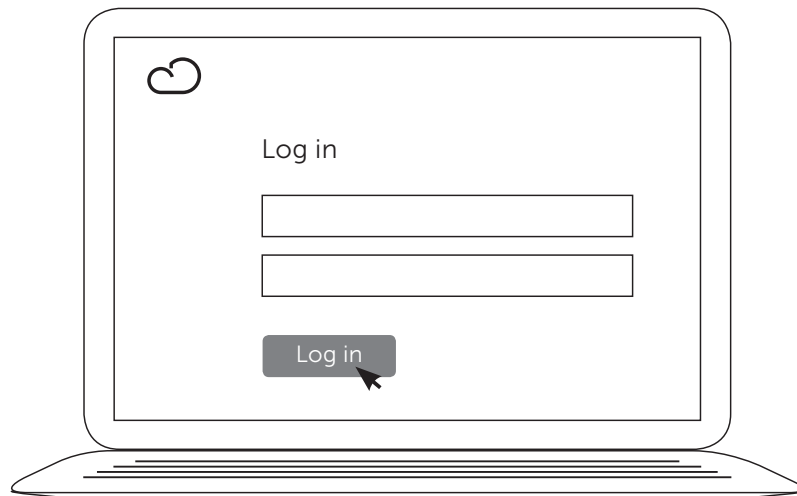

6

Attach cuff


Follow the on-screen instructions to properly put the cuff on your arm.



7

Take a reading


Press the start button to take a reading.

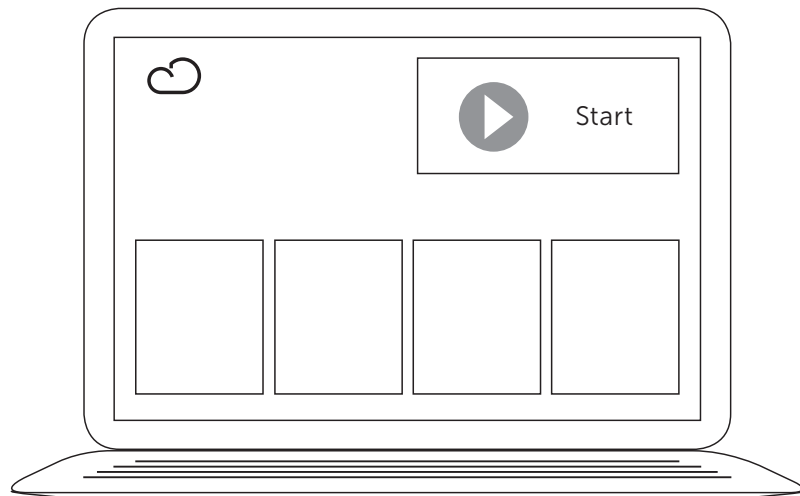

8

Install

If this is your first time you may be prompted to install our plug-in. If prompted, install required software and follow instructions on the screen. When completed, your Pulsewave® will be ready for use.

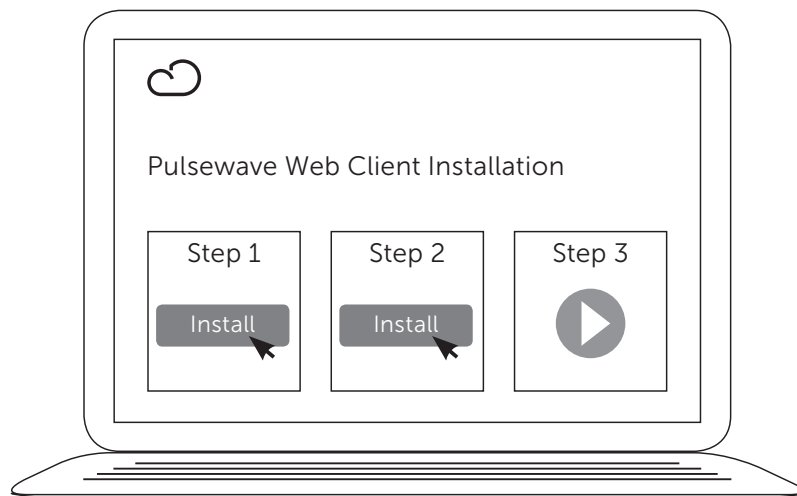

9

Support

Cloud DX maintains a convenient support web interface that includes an extensive knowledge base, describing all of the functions of Pulsewave®. Please explore the knowledge base here:

<https://support.clouddx.com>

For more information and to receive answers to your questions, please contact Cloud DX Support:

Telephone: **Toll Free: 1-888-543-0944 x1**

Email: **support@clouddx.com**

Hours: **Monday - Friday 9:00 - 17:00 Eastern Time**



Things to know

- ❖ Intended for use only by adults (18 years or older).
- ❖ Not intended to replace regular medical examinations.
- ❖ Do not adjust your medication, diet, or lifestyle without first consulting a physician.
- ❖ Do not use the cuff on skin with cuts, scrapes, open wounds etc.

Conditions that adversely affect use

- ❖ Temperature and relative humidity outside the specified operating range
(refer to Technical specifications at pulsewavedx.com)
 - ❖ Mechanical vibrations
 - ❖ Incorrect positioning of the cuff
(eg. placed too far up from the wrist, too loose or too tight)
 - ❖ Wrist not aligned at heart level
 - ❖ Any movement, including talking, during the reading
 - ❖ Your physiological condition (such as arrhythmias, and pregnancy)
-



 Manufactured by:

Cloud DX Inc.

#100 - 72 Victoria Street South
Kitchener ON
N2G 4Y9
clouddx.com



European Representative:
Advena Ltd., Pure Offices
Plato Close, Warwick CV34 6WE UK

Customer Support:
1-888-543-0944 ext 1
support@clouddx.com

© 2016 Cloud DX Inc

Version 4.2, SGPWEN42

FDA
CLEARED

HEALTH
CANADA
LICENSED

